



(A) System performance test solution\*  
(50 µg/mL Cetirizine dihydrochloride, 60 µg/mL Aminopyrine)

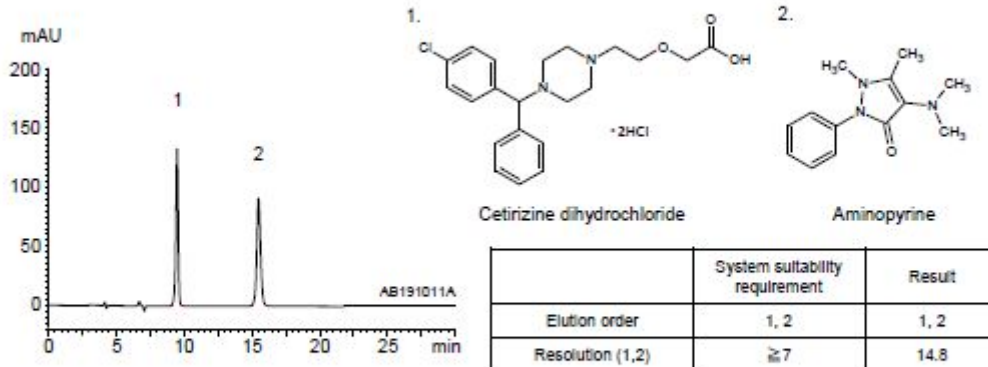

(B) Standard solution\*  
(4.0 µg/mL Cetirizine dihydrochloride)

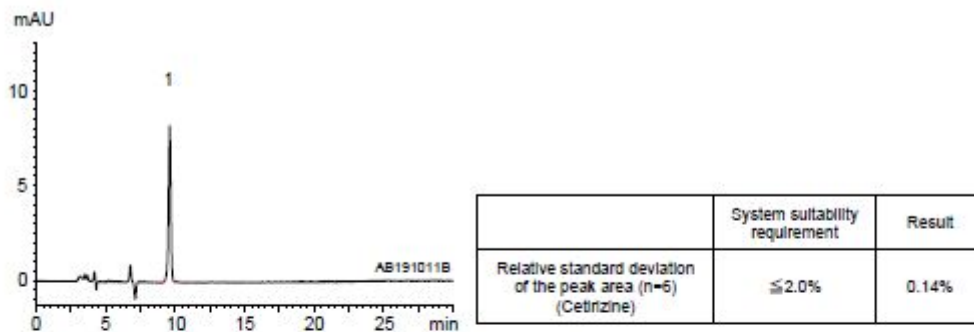

Column : YMC-Triart SIL (5 µm, 12 nm)  
250 X 4.0 mm I.D.

Eluent : acetonitrile/0.04 M sulfuric acid (94/6)

Flow rate : 0.75 mL/min (adjust the flow rate so that the retention time of Cetirizine is about 9 min)

Temperature : 25°C

Detection : UV at 230 nm

Injection : 10 µL

(The Japanese Pharmacopoeia 17th; Purity (2) Related substances)

\*All system performance test and standard solutions were prepared from Cetirizine dihydrochloride supplied as a reagent for laboratory use.