




System suitability solution *
 (0.3 mg/mL Losartan potassium, 0.002 mg/mL Triphenylmethanol)

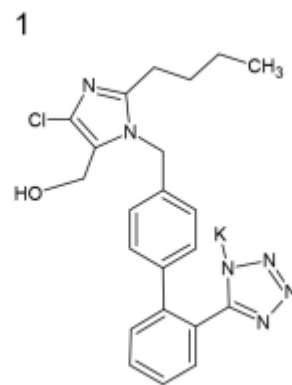

Losartan potassium



Triphenylmethanol

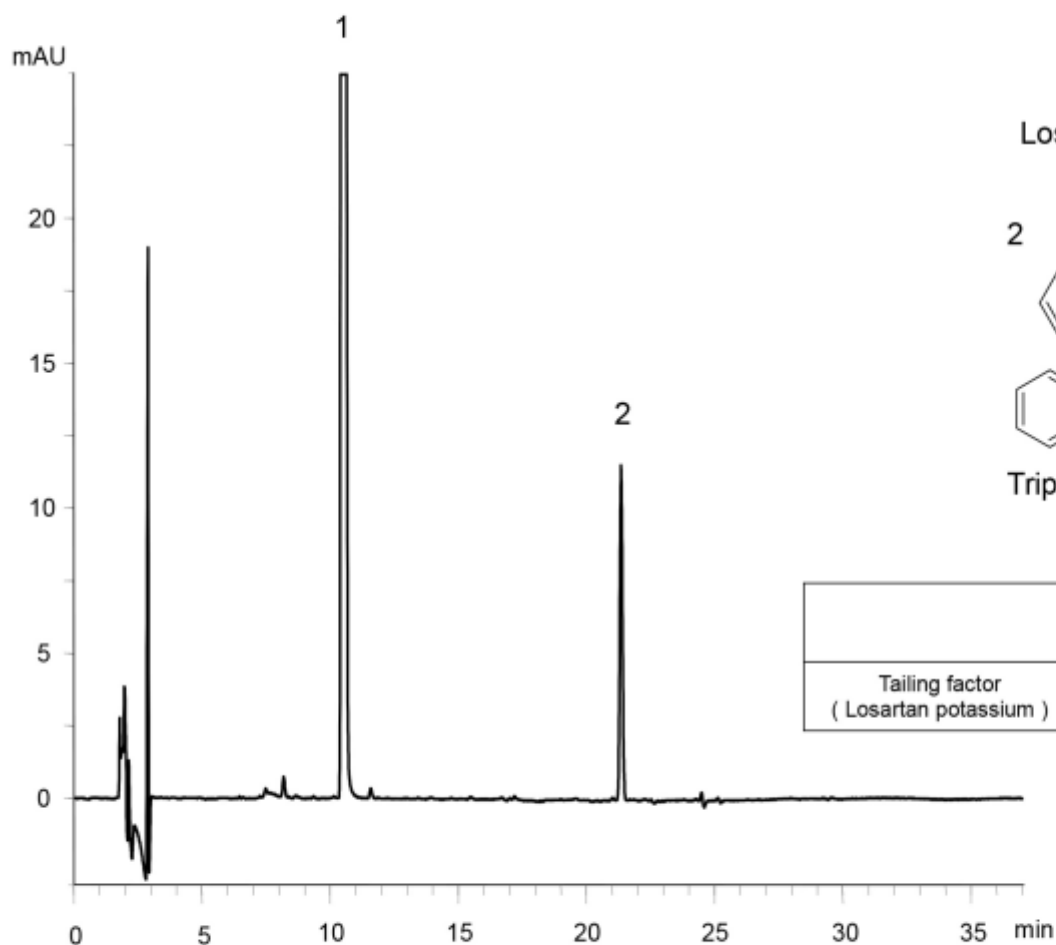

	System suitability requirement	Result
Tailing factor (Losartan potassium)	≤ 1.6	1.16

Column : YMC-Triart C18 (5 μ m, 12 nm)
 250 X 4.0 mmI.D.
 Eluent : A) 0.1% phosphoric acid
 B) acetonitrile
 25-90%B (0-25 min), 90%B (25-35 min)
 Flow rate : 1.0 mL/min
 Temperature : 25°C
 Detection : UV at 220 nm
 Injection : 10 μ L
 (The United States Pharmacopeia 34th; Chromatographic purity)

* System suitability solution was prepared from Losartan potassium supplied as a reagent for laboratory use.