




## Procedure




YMC-Triart C18 (5 µm, 250 X 4.6 mmI.D.)

Injection : 100 µL


Standard

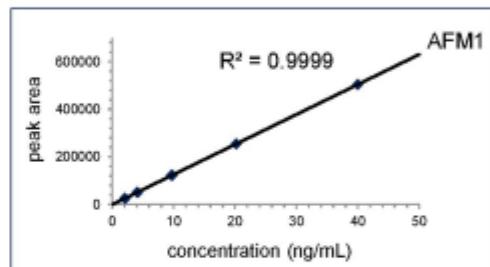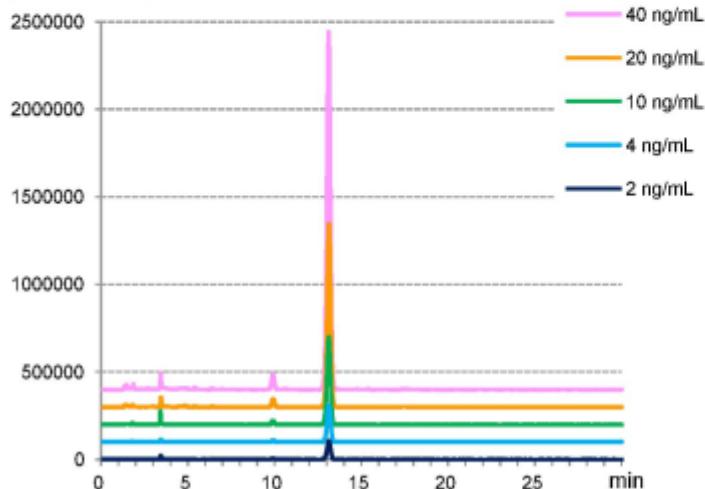


Matrix standard (10 ng/mL)

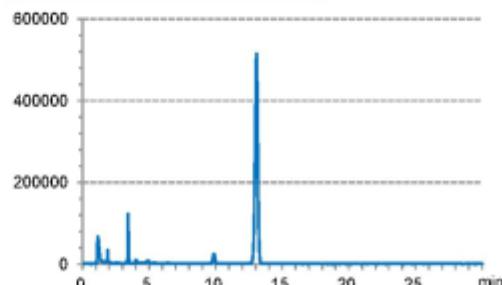

YMC-Triart C18 (5 µm, 250 X 4.6 mmI.D.)

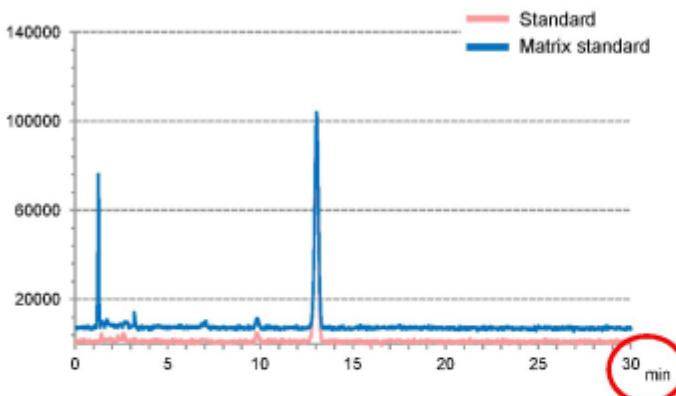

YMC-Triart C18 (3 µm, 100 X 3.0 mmI.D.)

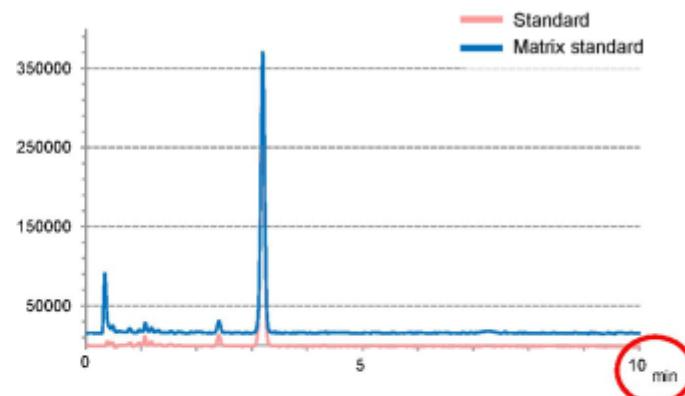

Courtesy of Japan Frozen Foods Inspection Corporation

Column	: YMC-Triart C18 (12 nm)
Eluent	: acetonitrile/water (25/75)
Flow rate	: 1.0 mL/min for 4.6 mmI.D., 0.8 mL/min for 3.0 mmI.D.
Temperature	: 40°C
Detection	: FLS at Ex 365 nm, Em 435 nm
Injection	: 20 µL