

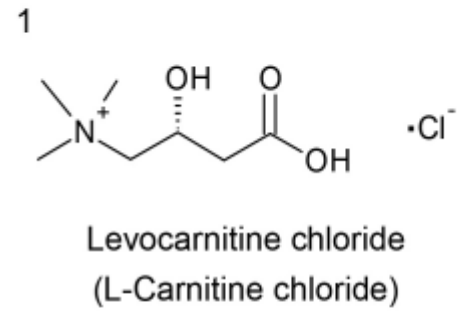
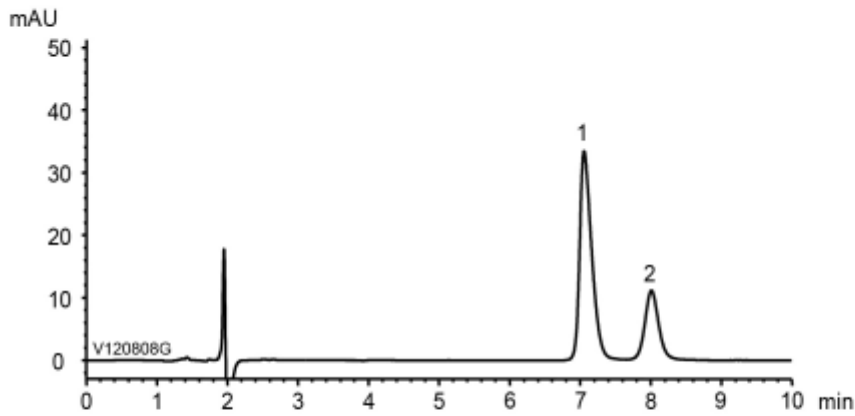


(A) Standard

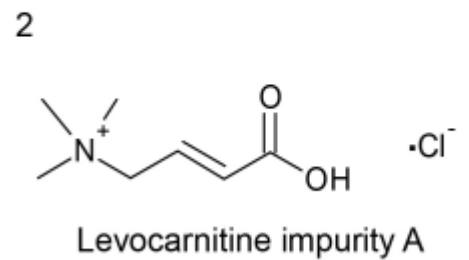

(B) Levocarnitine injection

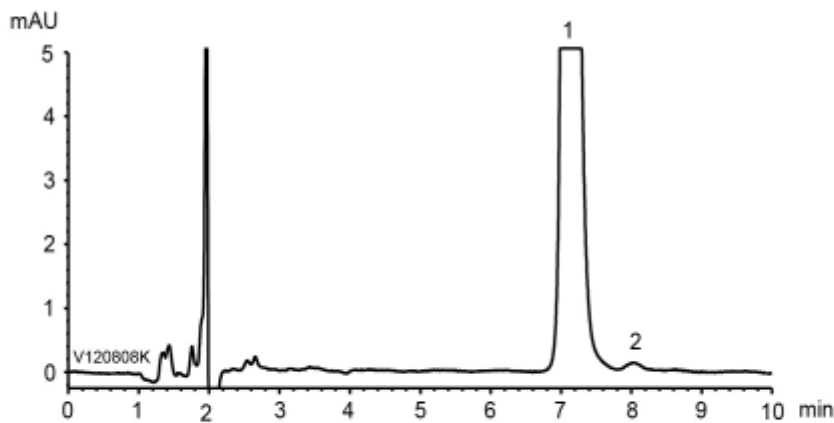

Column	: YMC-Triart Diol-HILIC (5 $\mu$ m, 12 nm) 150 X 4.6 mm I.D.
Eluent	: 50 mM KH <sub>2</sub> PO <sub>4</sub> -H <sub>3</sub> PO <sub>4</sub> (pH 4.3)/acetonitrile (25/75)
Flow rate	: 1.0 mL/min
Temperature	: 30°C
Detection	: UV at 205 nm
Injection	: 2 $\mu$ L
Sample	: (A) Standard (5 mg/mL, 0.025 mg/mL) (B) Levocarnitine injection diluted with acetonitrile/water (50/50) (correspond to 5 mg/mL Levocarnitine)